

Drug Tests Cup

Package Insert for testing of any combination of the following drugs:

AMP/BAR/BZO/BUP/COC/THC/MTD/MET/MDMA/MOP/OXY/PCP

One step, rapid screening tests for the qualitative detection of drug(s) and drug metabolite(s) in human urine.

For in vitro diagnostic use only.

INTENDED USE

Drug Tests Cup is a lateral flow chromatographic immunoassay designed to qualitatively detect the presence of drugs and drug metabolites in human urine at the following cut-off concentrations:

Test Name	Calibrator	Cut-off
Amphetamine/AMP	D-Amphetamine	1000 ng/mL
Barbiturates/BAR	Secobarbital	300 ng/mL
Benzodiazepines/BZO	Oxazepam	300 ng/mL
Buprenorphine/BUP	Buprenorphine	10 ng/mL
Cocaine/COC	Benzoylcegonine	300 ng/mL
Marijuana/THC	Delta-9-THC-COOH	50 ng/mL
Methadone/MTD	Methadone	300 ng/mL
Methamphetamine/mAMP/MET	D-Methamphetamine	1000 ng/mL
Methylenedioxyamphetamine/MDMA	MDMA	500 ng/mL
Opiates 300/Morphine/MOP	Morphine	300 ng/mL
Oxycodone/OXY	Oxycodone	100 ng/mL
Phencyclidine/PCP	Phencyclidine	25 ng/mL

Drug Tests Cup provides only a preliminary analytical test result. The test is not intended to be used in monitoring the drug levels. A more specific alternate method must be used in order to confirm the test result. Gas Chromatography/Mass Spectrometry (GC/MS) is the preferred confirmatory method. Clinical consideration and professional judgment should be applied to any drug of abuse test results, particularly when preliminary positive results are obtained.

SUMMARY AND EXPLANATION OF THE TEST

Drug Tests Cup is an easy, fast, qualitative, visually read competitive binding immunoassay method for screening specific drugs and their metabolites without the need of instrumentation. The method employs a unique mixture of antibodies to selectively detect the elevated levels of specific drugs and their metabolites in urine.

AMPHETAMINE / AMP

Amphetamines are central nervous system stimulants that produce alertness, wakefulness, increased energy, reduced hunger, and overall feeling of well-being. They are chemically related to the human body's natural catecholamines: epinephrine and norepinephrine. Large doses and extended usage can result in higher tolerance levels and physiological dependency leading to substance abuse. The effect of Amphetamines generally last 2-4 hours following use, and the drug has a half-life of 4-24 hours in the body. About 30% of Amphetamines are excreted in the urine in unchanged form, with the remainder as hydroxylated and deaminated derivatives. **Drug Tests Cup** yields a positive result when Amphetamines in urine exceed 1000 ng/mL, which is the suggested screening cut-off for positive specimens by the Substance Abuse and Mental Health Services Administration (SAMHSA, USA).

BARBITURATES / BAR

Barbiturates are central nervous system depressants. They are usually administered orally but are sometimes injected intramuscularly and intravenously. Barbiturates range from short-acting (approximately 15 minutes, such as secobarbital) to long-acting (24 hours or longer, such as Phenobarbital). Short-acting barbiturates are extensively metabolized in the body, while the long-acting ones are secreted primarily unchanged. Barbiturates produce alertness, wakefulness, increased energy, reduced hunger, and an overall feeling of well being. Large doses of Barbiturate could develop tolerance and physiological dependency and lead to its abuse. **Drug Tests Cup** yields a positive result when secobarbital in urine exceeds 300 ng/mL.

BENZODIAZEPINES / BZO

Benzodiazepines are a class of drugs that are often therapeutically used as anxiolytics, anti-convulsants and sedative hypnotics. Benzodiazepines manifest their presence by analgesia, drowsiness, confusion, diminished reflexes, lowering of body temperature, respiratory depression, blockade of adrenocortical response, and a decrease in peripheral resistance without an impact on the cardiac index. The major pathways of elimination are the kidneys (urine) and the liver where it is conjugated to glucuronic acid. Large doses of Benzodiazepines could develop tolerances and physiological dependency and lead to its abuse. Only trace amounts (less than 1%) of Benzodiazepines are excreted unaltered in the urine, most of Benzodiazepines in urine is conjugated drug. Oxazepam, a common metabolite of many benzodiazepines, remains detectable in urine for up to one week, which

makes Oxazepam a useful marker of Benzodiazepines abuse. **Drug Tests Cup** yields a positive result when oxazepam in urine exceeds 300 ng/mL.

BUPRENORPHINE / BUP

Buprenorphine is a potent analgesic often used in the treatment of opioid addiction. The drug is sold under the trade names Subutex™, Buprenex™, Temgesic™ and Suboxone™, which contain Buprenorphine HCl alone or in combination with Naloxone HCl. Therapeutically, Buprenorphine is used as a substitution treatment for opioid addicts. Substitution treatment is a form of medical care offered to opiate addicts (primarily heroin addicts) based on a similar or identical substance to the drug normally used. In substitution therapy, Buprenorphine is as effective as Methadone but demonstrates a lower level of physical dependence. Concentrations of free Buprenorphine and Norbuprenorphine in urine may be less than 1 ng/ml after therapeutic administration, but can range up to 20 ng/ml in abuse situations. The plasma half life of Buprenorphine is 2-4 hours. While complete elimination of a single dose of the drug can take as long as 6 days, the window of detection for the parent drug in urine is thought to be approximately 3 days. **Drug Tests Cup** yields a positive result when Buprenorphine in urine exceeds 10 ng/mL.

COCAINE / COC

Cocaine is an alkaloid present in Coca leaves (Erythroxine coca). Its pharmacological properties, such as stimulating and euphoric effects, have been known for centuries. Cocaine produces alertness, wakefulness, increased energy, reduced hunger, and an overall feeling of well being. In large dose, Cocaine causes fever, unresponsiveness, difficulty in breathing and unconsciousness. Cocaine is often self-administered by nasal inhalation, intravenous injection and free-base smoking. Cocaine is excreted in the urine primarily as Benzoylcegonine, which can generally be detected for 24 – 48 hours after cocaine exposure. **Drug Tests Cup** yields a positive result when the Cocaine metabolite in urine exceeds 300 ng/mL, which is the suggested screening cut-off for positive specimens set by the Substance Abuse and Mental Health Service Administration (SAMHSA, USA).

MARIJUANA / THC

THC (Δ^9 – tetrahydrocannabinol) is the primary active ingredient in cannabis (marijuana). THC is central nervous stimulant that alters mood and sensory perceptions, produces loss of coordination, impairs short-term memory, produces symptoms of anxiety, paranoia, depression, confusion, hallucination, and increases heart rate. Large doses of marijuana could develop tolerances and physiological dependency and lead its abuse. The main metabolite excreted in the urine is 11-nor- Δ^9 – tetrahydrocannabinol-9-carboxylic acid (Δ^9 -THC-COOH), which is found in the urine within hours of exposure and remains detectable for 3-10 days after smoking. **Drug Tests Cup** yields a positive result when the concentration of THC-COOH in urine exceeds 50 ng/mL, which is the suggested screening cut-off for positive specimens set by the Substance Abuse and Mental Health Service Administration (SAMHSA, USA).

METHADONE / MTD

Methadone is a narcotic analgesic prescribed for the management of moderate to severe pain and for the treatment of opiate dependence (Heroin, Vicodin, Percocet, Morphine). It is administered either orally, or by intravenous or intra-muscular injection. The duration of effect of methadone is 12 – 24 hours. Its major urinary excretion products are methadone, EDDP (2-ethylidene-1,5-dimethyl-3,3-diphenylpyrrolidine), and EMDP (2-ethyl-5-methyl-3,3-diphenylpyrrolidine). **Drug Tests Cup** yields a positive result when the concentration of Methadone in urine exceeds 300 ng/mL.

METHAMPHETAMINE / mAMP / MET

Methamphetamine is an addictive stimulant drug that strongly activates certain systems in the brain. Methamphetamine is closely related chemically to amphetamine, but the central nervous system effects of methamphetamine are greater. Methamphetamine can be taken orally, injected, or inhaled. Acute higher doses lead to enhanced stimulation of the central nervous system and induce euphoria, alertness, reduced appetite, and a sense of increased energy and power. Methamphetamine is excreted in the urine as amphetamine and oxidized and deaminated derivatives. However, 10 to 20 % of Methamphetamine is excreted unchanged. Thus, the presence of the parent compound in the urine indicates Methamphetamine use. **Drug Tests Cup** yields a positive result when the concentration of Methamphetamine in urine exceeds 1000 ng/mL.

METHYLENEDIOXYMETHAMPHETAMINE / MDMA

MDMA belongs to a family of man-made drugs. Its relatives include MDA (methylenedioxyamphetamine), and MDEA (methylenedioxyethylamphetamine). They all share the amphetamine-like effects. MDMA is a stimulant with hallucinogenic tendencies described as an empathogen as it releases mood-altering chemicals, such as cartooning and L-dopa, and may generate feelings of love and friendliness. The adverse effects of MDMA use include elevated blood pressure, hyperthermia, anxiety, paranoia and insomnia. MDMA

is administered either by oral ingestion or intravenous injection. The effects of MDMA begin 30 minutes after intake, peak in an hour and last for 2 – 3 hours. **Drug Tests Cup** yields a positive result when the concentration of MDMA in urine exceeds 500 ng/mL.

OPIATES 300 / MOP

Opiates refer to any drug that is derived from the opium poppy, including the natural products, morphine and codeine, and the semi-synthetic drugs such as heroin. Opiates exert their effects on the central nervous system and organs containing smooth muscle. Opiates manifest their presence by analgesia, drowsiness, euphoria, lowering of body temperature, respiratory depression, blockade of adrenocortical response. The major pathways of elimination are kidneys (urine) and the liver where it is conjugated to glucuronic acid. Opiates and their metabolites can be detected in urine as result of heroin, morphine, codeine or poppy seed intake. **Drug Tests Cup** yields a positive result when the concentration of Opiates in urine exceeds 300 ng/mL.

OXYCODONE / OXY

Oxycodone is an analgesic, which works by depressing the central nervous system. Oxycodone is abused for its opiate-like effects. In addition to its equal potency to morphine in analgesic effects, it is also equipotent to morphine in relieving abstinence symptoms from chronic opiate (heroin, morphine) use. For this reason, it is often used to alleviate or prevent the onset of opiate withdrawal by street users of heroin and methadone. The drug is most often administered orally. Like other opiates, Oxycodone can also depress the respiratory system resulting in suffocation and death when overdosed. Oxycodone is very addictive, both physically and psychologically. Some physical indications of Oxycodone abuse include extreme loss of appetite and weight, cramps, nausea, vomiting, excessive scratching and complaint of itching, excessive sweating, constipation, pin-point pupils and watery eyes, reduced vision, drowsiness, euphoria, trance-like states, excessive thirst, tremors, twitching, irritability, hallucinations and lethargy. **Drug Tests Cup** yields a positive result when the concentration of Oxycodone in urine exceeds 100 ng/mL.

PHENCYCLIDINE / PCP

Phencyclidine, commonly known as PCP or “angel dust” is used primarily as recreational drug due to its hallucinogenic effects. It is generally self-administered by intravenous injection or by inhalation and concentrates fastest in fatty tissues and the brain. The effects of PCP are very much dose related. Small amounts of Phencyclidines (PCP) are central nervous system stimulants that produce alertness, wakefulness, increased energy, increased heat rate, and decreased sense of pain and touch, and an overall feeling of well being. Large doses of Phencyclidine (PCP) can result in death due to convulsions, heart and lung failure and coma. Large repeated doses of Phencyclidine (PCP) could develop tolerances and physiological dependency and lead to its abuse. PCP can be found in urine within 4 to 6 hours after use and will remain in urine for 7 to 14 days. Phencyclidine is excreted in the urine as an unchanged drug (4% to 19%) and conjugated metabolites (25% to 30%). **Drug Tests Cup** yields a positive result when the concentration of Phencyclidine in urine exceeds 25 ng/mL, which is the suggested screening cut-off for positive specimens set by the Substance Abuse and Mental Health Service Administration (SAMHSA, USA).

PRINCIPLE OF TEST

Drug Tests Cup is a competitive binding immunoassay in which drugs and drug metabolites in a urine sample compete with immobilized drug conjugate for limited labeled antibody binding sites. When a sufficient amount of urine specimen is applied to the sample pad of the test device, the urine specimen migrates through the test device by capillary action. If the drug or drug metabolite concentration in the specimen is below the cut-off level, the anti-drug antibodies in colloidal gold particles will bind to the drug antigens coated in the test line of the nitrocellulose membrane to form a T line, which indicates a negative result. If the concentration of drug in the urine specimen is above the cut-off level, it will bind with antibodies conjugated with colloidal gold particles, so that no T line will be developed in the test region, which indicates a positive result.

REAGENTS

Drug Tests Cup contains membrane strips coated with drug-protein conjugates (purified bovine albumin) on the T zone, goat polyclonal antibody against gold-protein conjugate at the C zone, and a dye pad which contains colloidal gold particles coated with mouse monoclonal antibodies specific against Amphetamine, Barbiturates, Benzodiazepines, Buprenorphine, Cocaine, Marijuana, Methadone, Methamphetamine, Methylenedioxyamphetamine, Morphine, Oxycodone and Phencyclidine.

MATERIALS PROVIDED

- Drug Tests Cup
- Product insert
- Security Seal
- Procedure Card

MATERIALS REQUIRED BUT NOT PROVIDED

- Clock or timer
- External positive and negative controls

PRECAUTIONS

1. For *in vitro* diagnostic use only.
2. Do not use after the expiration date.
3. The drug tests should remain in the sealed pouch until use.
4. All specimens should be considered potentially hazardous and handle in the same way as an infectious material.
5. All used drug tests should be discarded according to federal, state and local regulation.

STORAGE AND STABILITY

Store **Drug Tests Cup** in the sealed pouch at 2°C to 30°C. The drug tests is stable through the expiration date printed on the sealed pouch. The drug tests must remain in the sealed pouch until use. If store at 2°C to 8°C, allow the drug tests to reach room temperature (15°C to 30°C) before performing the test. Do not freeze, do not use beyond the expiration date.

SPECIMEN COLLECTION AND STORAGE


Fresh urine specimens should be collected directly into a clean and dry container. Urine collected at any time of the day may be used for testing. Urine specimen exhibiting visible precipitates should be centrifuged, filtered or allowed the precipitates to settle to obtain a clear specimen for testing. For best results, test a fresh specimen immediately following collection. Storage of specimens should not exceed 2 hours at room temperature or 4 hours refrigerated (2-8°C) prior to using.

TEST PROCEDURE

For Drug Test Cup:

Allow the cup, urine specimen (if refrigerated), and/or controls to equilibrate to room temperature (15-30°C) prior to testing.

1. Remove the cup from the sealed pouch and use it as soon as possible.
2. Collect specimen in the cup and secure the cap tightly.
3. If the temperature strip is included with Drug Test Cup, please read urine temperature between 2-4 minutes after voiding to verify the temperature ranges between 90-100°F (33-38°C).
4. Place the cup on a flat surface.
5. Date and initial the security seal, and place the security seal on the cap.
6. Peel off the label on the cup to view the results.
7. **Read the test results at 5 minutes.** See the illustration below. For detailed operation instructions, please refer to the Procedure Card.

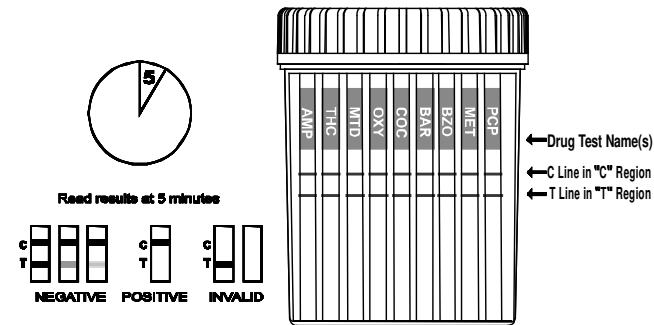

INTERPRETATION OF RESULTS

Positive: One colored line appears in the Control zone (C). No line appears in the Test zone (T). The absence of a line in the test region (T line) indicates a positive result. The positive result indicates that the drug level is above the detectable level.

Note: The samples with positive results should be confirmed with more specific method.

Negative: One colored line appears in the Control zone, and another colored line appears in the Test zone. The negative result indicates the drug or its metabolite level is below the detectable level.

Invalid: No line appears in the Control zone. If no C line or no C line and T line develop within 5 to 10 minutes, the test is invalid. The test should be repeated with a new test device. Insufficient specimen volume or the incorrect procedural techniques are the most likely reasons for invalid result. Review the procedure and repeat the test using a new test strip or device. If the problem persists, discontinue using the current lot and contact your suppliers.

QUALITY CONTROL

1. Built-in Control: the test contains a built-in control feature, the C line. The presence of the C line indicates that the test is performed properly. If a C line does not form, the test is considered invalid. In this case, the testing should be repeated with a new drug test.
2. External Quality Control: Control materials are not supplied with this kit. However, it is recommended that positive and negative controls should be tested as good laboratory practice to confirm the test procedure and to verify proper test performance.
3. Test each new lot and shipment by using external quality control materials (positive and negative), with each new untrained operator, monthly for storage, and as otherwise required by your lab internal quality system procedures.

LIMITATIONS

1. **Drug Tests Cup** provides only a qualitative, preliminary testing result. A more specific testing method must be used in order to obtain a confirmed testing result. Gas Chromatography/Mass Spectrometry (GC/MS) is the preferred confirmatory method.
2. There is a possibility that technical or procedural errors, as well as other interfering substances in the urine specimen may cause erroneous results.
3. Adulterants such as bleach or other oxidizing agents may produce erroneous results. If suspected, the test should be repeated with a fresh specimen and a new drug tests.
4. The urine specimens with bacterial contamination should not be used for testing, as these contaminations may interfere with the test and cause false results.
5. A positive result does not indicate the level of intoxication, the route of the drug administration or the concentration of the drug in the urine.
6. A negative result may not necessarily indicate drug-free urine. Negative results can be obtained when drug is present but below the cut-off level of test.
7. Test does not distinguish between drugs of abuse and certain medications.
8. Certain foods or food supplements may cause a false positive result.

PERFORMANCE CHARACTERISTICS

Accuracy:

The comparison studies were conducted using **Drug Tests Cup** and commercially available rapid drugs of abuse tests. The studies were performed on approximately 128 clinical specimens per drug type previous collected from the clinical settings. Presumptive positive results were confirmed by GC/MS. The following results are summarized from these comparison studies:

	% Agreement with Commercial Kit								
	AMP	BAR	BZO	BUP	COC	THC	MTD	MET	MDMA
Positive Agreement	100%	98%	97%	100%	100%	100%	98%	100%	97%
Negative Agreement	98%	98%	97%	100%	100%	98%	97%	98%	97%
Total Agreement	99%	98%	97%	100%	100%	99%	97.5%	99%	97%

	MOP	OXY	PCP
Positive Agreement	100%	98%	100%
Negative Agreement	100%	98%	98%
Total Agreement	100%	98%	99%

	% Agreement with GC/MS								
	AMP	BAR	BZO	BUP**	COC	THC	MTD	MET	MDMA
Positive Agreement	100%	98%	97%	95%	100%	100%	98%	100%	97%
Negative Agreement	98%	98%	97%	100%	100%	98%	97%	98%	97%
Total Agreement	99%	98%	97%	97.5%	100%	99%	97.5%	99%	97%

	MOP	OXY	PCP
Positive Agreement	100%	98%	100%
Negative Agreement	100%	98%	98%
Total Agreement	100%	98%	99%

BUP**: BUP was based on LC/MS data.

Sensitivity:

Sensitivity of **Drug Tests Cup** was characterized by validating the test performance around

the claimed cut-off concentration of each test. The cut-off of each test was determined by the lowest concentration of drug which produces at least 50% positive testing results in total numbers of determinations. The results were summarized as the following:

Drug concentration Cut-off Range	n	AMP		BAR		BZO		BUP	
		-	+	-	+	-	+	-	+
0% Cut-off	20	20	0	20	0	20	0	20	0
-50% Cut-off	20	20	0	20	0	20	0	20	0
-25% Cut-off	20	20	0	20	0	20	0	20	0
+25% Cut-off	20	1	19	0	20	0	20	0	20
+50% Cut-off	20	0	20	0	20	0	20	0	20

Drug concentration Cut-off Range	n	COC		THC		MTD		MET	
		-	+	-	+	-	+	-	+
0% Cut-off	20	20	0	20	0	20	0	20	0
-50% Cut-off	20	20	0	20	0	20	0	20	0
-25% Cut-off	20	20	0	20	0	20	0	20	0
+25% Cut-off	20	7	13	2	18	1	19	0	20
+50% Cut-off	20	0	20	0	20	0	20	0	20

Drug concentration Cut-off Range	n	MDMA		MOP		OXY		PCP	
		-	+	-	+	-	+	-	+
0% Cut-off	20	20	0	20	0	20	0	20	0
-50% Cut-off	20	20	0	20	0	20	0	20	0
-25% Cut-off	20	20	0	20	0	20	0	20	0
+25% Cut-off	20	0	20	0	20	3	17	5	15
+50% Cut-off	20	0	20	0	20	0	20	0	20

Based on above data, sensitivity of the assay to the 12 analytes is as follows:

Amphetamine:	1000 ng/mL	Methadone:	300 ng/mL
Barbiturates:	300 ng/mL	Methamphetamine:	1000 ng/mL
Benzodiazepines:	300 ng/mL	MDMA:	500 ng/mL
Buprenorphine:	10 ng/mL	Opiates 300:	300 ng/mL
Cocaine:	300 ng/ mL	Oxycodone:	100 ng/mL
Marijuana:	50 ng/mL	Phencyclidine:	25 ng/mL

Precision / Reproducibility:

Reproducibility was determined by replicating tests on five different concentrations of each drug in urine specimens: negative, 50% below cut-off, 25% below cut-off, 25% above cut-off and 50% above cut-off. Each drug test was tested four times daily for five consecutive days with a total 20 assays at each concentration. The data are summarized below:

Amphetamine Precision /Reproducibility Study:

Amphetamine Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
500	20	20/0	100%
750	20	20/0	100%
1250	20	1/19	95%
1500	20	0/20	100%

Barbiturates Precision/Reproducibility Study:

Barbiturates Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
150	20	20/0	100%
225	20	20/0	100%
375	20	0/20	100%
450	20	0/20	100%

Benzodiazepines Precision/Reproducibility Study:

Benzodiazepines Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
150	20	20/0	100%
225	20	20/0	100%
375	20	0/20	100%
450	20	0/20	100%

Buprenorphine Precision/Reproducibility Study:

Buprenorphine Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
5	20	20/0	100%
7.5	20	20/0	100%
12.5	20	1/19	95%
15	20	0/20	100%

Cocaine Precision/Reproducibility Study:

Cocaine Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%

150	20	20/0	100%
225	20	20/0	100%
375	20	7/13	65%
450	20	0/20	100%

Marijuana Precision/Reproducibility Study:

Marijuana Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
25	20	20/0	100%
37.5	20	20/0	100%
62.5	20	2/18	90%
75	20	0/20	100%

Methadone Precision/Reproducibility Study:

Methadone Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
150	20	20/0	100%
225	20	20/0	100%
375	20	1/19	95%
450	20	0/20	100%

Methamphetamines Precision/Reproducibility Study:

Methamphetamines Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
500	20	20/0	100%
750	20	20/0	100%
1250	20	0/20	100%
1500	20	0/20	100%

MDMA Precision/Reproducibility Study:

MDMA Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
250	20	20/0	100%
375	20	20/0	100%
625	20	0/20	100%
750	20	0/20	100%

Opiates 300 Precision/Reproducibility Study:

Opiates 300 Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
150	20	20/0	100%
225	20	20/0	100%
375	20	0/20	100%
450	20	0/20	100%

Oxycodone Precision/Reproducibility Study:

Oxycodone Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
50	20	20/0	100%
75	20	20/0	100%
125	20	3/17	85%
150	20	0/20	100%

Phencyclidine Precision/Reproducibility Study:

Phencyclidine Concentration (ng/mL)	Total numbers of Determinations	Results #Neg/#Pos	Precision (%)
0	20	20/0	100%
12.5	20	20/0	100%
18.75	20	20/0	100%
31.25	20	5/15	75%
37.5	20	0/20	100%

The data presented here demonstrates excellent precision/ reproducibility of **Drug Tests Cup** across multiple concentrations of human urine.

Analytical Specificity:

Cross-reactivity was established by spiking various concentrations of similarly structured drug compounds into drug-free urine /a negative control. Analyzing various concentration of each compound by using **Drug Tests Cup**, the concentration of the drug that produced a response approximately equivalent to the cut-off concentration of the assay was determined. Results of those studies appear in the table(s) below:

Drug Compound	Response equivalent to cutoff in ng/mL
AMPHETAMINE (AMP)	
D-Amphetamine	1000
D,L-Amphetamine	2500
L-Amphetamine	50000
(±)3,4-Methylenedioxyamphetamine (MDA)	2000
Ephedrine	>100000
3,4-Methylenedioxyamphetamine (MDEA)	>100000

BARBITURATES (BAR)	
Secobarbital	300
Phenobarbital	2500
Butalbital	500
Pentobarbital	1500
Amobarbital	2500
Cyclopentobarbital	500
Butethal	800
Barbital	300
Butabarbital	1500
BENZODIAZEPINES (BZO)	
Oxazepam	300
Alprazolam	200
α-Hydroxyvalprazolam	1000
Bromazepam	250
Chlordiazepoxide	2500
Clobazam	100
Clonazepam	850
Clorazepate	250
Delorazepam	1600
Diazepam	200
Estazolam	200
Flunitrazepam	300
Lorazepam	1000
Midazolam	1500
Nitrazepam	100
Nordiazepam	400
Temazepam	150
Triazolam	500
BUPRENORPHINE (BUP)	
Buprenorphine	10
Norbuprenorphine	15
Buprenorphine-3-D-glucuronide	12.5
Norbuprenorphine-3-D-glucuronide	175
Morphine-3-D-glucuronide	100000
Morphine	>100000
Oxymorphone	>100000
Hydromorphone	>100000
COCAINE (COC)	
Cocaine	>100000
Benzoylcegonine	300
Egonine HCl	35000
MARIJUANA (THC)	
11-nor-Δ ⁹ -THC-9-COOH	50
11-nor-Δ ⁹ -THC-9-COOH	50
Δ ⁹ -Tetrahydrocannabinol	8000
Δ ⁹ -Tetrahydrocannabinol	10000
Cannabidiol	10000
Cannabidiol	100000
METHADONE (MTD)	
Methadone	300
(±)2-Ethyl-1,5-dimethyl-3,3-diphenylpyrrolinium	50000
Doxylamine	50000
METHAMPHETAMINES (MET)	
+/-Methamphetamine	2000
+Methamphetamine	1000
3,4-Methylenedioxyethylamphetamine(MDEA)	35000
(+/-)3,4-Methylenedioxyamphetamine (MDMA)	2000
Ranitidine(Zantac)	>100000
3,4-Methylenedioxyamphetamine (MDA)	>100000
D-Amphetamine	>100000
L-Amphetamine	>100000
Ephedrine	>100000
METHYLENEDIOXYMETHAMPHETAMINE (MDMA)	
(+/-)3,4-Methylenedioxyamphetamine (MDMA)	500
D-Amphetamine	>100000
L-Methamphetamine	100000
3,4-Methylenedioxyethylamphetamine (MDEA)	200
3,4-Methylenedioxyamphetamine (MDA)	2000
OPIATE 300 (MOP)	
Morphine	300
Codeine	300
Hydrocodone	2000
Hydromorphone	3500
Morphine 3-β-D-glucuronide	300
6-Monoacetylmorphine	600
Normorphone	100000
Oxycodone	10000
Oxymorphone	50000
Thebaine	7000
OXYCODONE (OXY)	
Oxycodone	100
Morphine	50000

Codeine	25000
Morphine 3-β-D-glucuronide	50000
Hydrocodone	1600
Hydromorphone	15000
Normorphone	100000
Oxymorphone	1500
PHENCYCLIDINE (PCP)	
Phencyclidine	25
4-Hydroxyphencyclidine	15000

Interfering Compounds:

The following compounds in both drug-free urine and drug positive urines with Amphetamine, Barbiturate, Benzodiazepine, Buprenorphine, Cocaine, Marijuana, Methadone, Methamphetamines, Mehtylenedioxyamphetamine, Morphine, Oxycodone, Phencyclidine, show no cross-reactivity when tested with **Drug Tests Cup** at a concentration of 100 µg/mL.

Common Substances:

Acetaminophen	Diphenhydramine	(+/-)-Norephedrine
Acetone	Dopamine	Oxalic Acid
Albumin	(+/-)-Epinephrine	Penicillin-G
Ampicillin	Erythromycin	Pheniramine
Ascorbic Acid	Ethanol	Phenothiazine
Aspartame	Furosemide	1-Phenylephrine
Aspirin	Glucose	β-Phenylethylamine
Atropine	Guaiacol Glyceryl Ether	Procaine
Benzocaine	Hemoglobin	Quinidine
Bilirubin	Ibuprofen	Ranitidine
Caffeine	(+/-)-Isoproterenol	Riboflavin
Chloroquine	Ketamine	Sodium Chloride
(+)-Chlorpheniramine	Levorphanol	Sulindac
(+/-)-Chlorpheniramine	Lidocaine	Theophylline
Creatine	(+)-Naproxen	Tyramine
Dextrompheniramine	Niacinamide	4-Dimethylaminoantipyrine
Dextromethorphan	Nicotine	(1R,2S)-(-)-N-Methyl-Ephedrine

Biological Materials:

Albumin	Vitamin(L-Ascorbic Acid)
Bilirubin	Uric Acid
Creatine	Urine pH 4.5-9.0
Hemoglobin	Urine Specific Gravity 1.002-1.035 g/mL
Glucose	

(There is a possibility that other substances and/or factors not listed above may interfere with the test and cause false results.)

Bibliography:

- Baselt, R.C. Disposition of Toxic Drugs and Chemicals in Man, 4thEd., Biomedical Publ., Davis, CA., 1995.
- Department of Health and Human Service, Mandatory Guidelines for Federal Workplace Drug Testing Program, Fed Register. 53(69): 11970-11979, 1988.
- Gilman, A. G., and Goodman, L.S., The pharmacological basis of therapeutics, Ed. MacMillan Publishing, New York, NY, 1980.
- Urine Testing for Drugs of Abuse. National Institute on Drug Abuse (NIDA): Research Monograph, 73, 1986.
- Wilson, John, Abused Drugs II, a laboratory Pocket Guide. AACCPress. Washington, DC; 1994.
- Cody, J.T., "Specimen Adulteration in drug urinalysis. Forensic Sci. Rev., 1990, 2:63.
- Tsai, S.C. et al., J. Anal. Toxicol. 1998; 22 (6): 474.
- Tietz NW. Textbook of Clinical Chemistry.W.B.Saunders Company.1986;1735.

Revised: Sep, 2019